


<b>Individual Report</b>		<b>QCMD 2020 SARS-CoV-2 EQA Programme</b>					
<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023	

### Intended Results / Panel Composition

Sample Code	Sample Content	Matrix	Sample Relationships <sup>[1]</sup>	Detection Frequency <sup>[2]</sup>	Sample Status <sup>[3]</sup>	Percentage Correct (All) <sup>[4]</sup>	
						(%)	(n)
SCV2_101C2-01	Coronavirus OC43	Transport Medium	4.0 dPCR Log10 Copies/ml	Negative	CORE	97.8	451
SCV2_101C2-02	SARS-CoV-2	Transport Medium	3.27 dPCR Log10 Copies/ml (DS1_1)	Frequently Detected	CORE	98.7	451
SCV2_101C2-03	SARS-CoV-2	Transport Medium	2.48 dPCR Log10 Copies/ml (D1, DS1_2)	Detected	CORE	93.1	451
SCV2_101C2-04	SARS-CoV-2	Transport Medium	2.48 dPCR Log10 Copies/ml (D1, DS1_2)	Detected	CORE	93.6	451
SCV2_101C2-05	Coronavirus Negative	Transport Medium		Negative	CORE	99.1	451

**[1] Sample Relationships:** Indicates the relationships of the samples within this challenge. The highest titre member of dilution series DS1 is indicated by DS1\_1 and further members of the series as DS1\_2, DS1\_3 etc. in order of reducing titre. Additional dilution series are indicated by DS2 (e.g DS2\_1, DS2\_2 etc.), DS3 (e.g. DS3\_1, DS3\_2 etc.). If one duplicate pair is present this is indicated by 'D1'. Further duplicate pairs are indicated by 'D2', 'D3' etc.

**[2] Detection Frequency:** To aid qualitative analysis each panel member is assigned a frequency of detection. This is based on the peer group consensus of all qualitative results returned from participants within the EQA challenge / distribution.

**[3] Sample Status:** EQA samples are defined as "CORE" or "EDUCATIONAL". Core proficiency samples are reviewed by the QCMD Scientific Expert(s). This is on the basis of scientific information, clinical relevance, current literature and, where appropriate, professional clinical guidelines. Participating laboratories are expected to report core proficiency samples correctly within the EQA challenge / distribution.

**[4] Percentage Correct (All):** Percentage of datasets (%) reporting the correct qualitative result and the total number of datasets (n) reported for each panel member.

*For further details please refer to the current participant manual.*

**[1] Sample Relationships:** Includes dPCR Log10 Copies/ml, the value obtained using a digital droplet PCR assay (modified from Eurosurveillance Jan 2020 Corman et al).

**Please note:** The values provided are for reference only. The values obtained by individual participating laboratories will vary from the dPCR values provided. This is because quantitation is dependent on the molecular workflow each laboratory uses (i.e. nucleic acid extraction and molecular platform / assay) as well as the standards or reference material used to calibrate the molecular workflow. In the absence of an International Standard or Certified Reference Material (CRM), QCMD uses Internal Reference Materials (IRMs) with values established using a dPCR reference assay in order to support the consistency and traceability of the EQA materials. This also helps aid the comparison of results across laboratories.


### Your Summary Results

**EQA Assessment Group <sup>[1]</sup>**

GeneProof SARS-CoV-2

**Core Panel Detection (Qualitative) Score <sup>[2]</sup>**

0

<b>Individual Report</b>		<b>QCMD 2020 SARS-CoV-2 EQA Programme</b>				 <small>Quality Control for Molecular Diagnostics</small>	
<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023	

### Core Panel Members Results

Sample Code	Qualitative Results			Your Quantitative Data (for information only) <sup>[3]</sup>		
	Percentage Correct (All) <sup>[4]</sup>	Your Result <sup>[5]</sup>	Detection Score <sup>[6]</sup>	Reported Value	Unitage	Cycle Threshold
SCV2_101C2-01	97.8	Negative	0		N/A	-
SCV2_101C2-02	98.7	Positive	0		N/A	29.13
SCV2_101C2-03	93.1	Positive	0		N/A	34.74
SCV2_101C2-04	93.6	Positive	0		N/A	34.4
SCV2_101C2-05	99.1	Negative	0		N/A	-

[1] **EQA Assessment Group:** To aid data analysis, participant results are grouped according to the molecular amplification/detection method specified within their molecular workflow for this challenge / distribution. For further details refer to the *Additional Information: Individual Panel Member Analysis* section of this report.

[2] **Core Panel Detection (Qualitative) Score:** An overall core panel detection score provided per challenge / distribution.

[3] **Quantitative Data (for information only):** This is the quantitative value, unitage and cycle threshold you provided when you submitted your results. For qualitative programmes this information is not used as part of your formal EQA assessment.


[4] **Percentage Correct (All):** Percentage of datasets (%) reporting the correct qualitative results for each panel member.


[5] **Your Result:** The qualitative result you reported for each sample within this EQA challenge / distribution.

[6] **Detection Score:** Your detection (qualitative) scores are based on the assigned detection frequency of each panel members, where 0 (zero) is "highly satisfactory" and 3 (three) is "highly unsatisfactory". Scores are provided for individual panel members.

**For further details please refer to the current participant manual.**

### Core Panel Member Score Breakdown

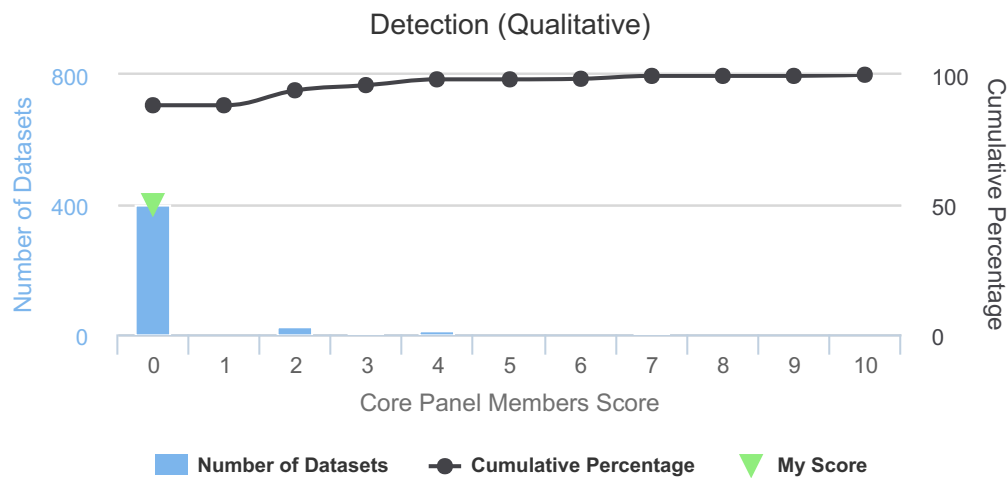




<b>Individual Report</b>		<b>QCMD 2020 SARS-CoV-2 EQA Programme</b>			 <small>Quality Control for Molecular Diagnostics</small>	
<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023

**Core Panel Member Score Breakdown - Detection:** This figure gives you a breakdown of the qualitative detection scores for all qualitative datasets returned within this EQA challenge / distribution independent of the EQA assessment group. Panel detection scores are generated from only those panel members that are defined as "CORE".

*For further details please refer to the current participant manual.*

## My Workflow Details

The details of the workflow(s) used to submit your results for this challenge.


<b>Name</b>	SARS-CoV-2 PCR Kit (v4)
<b>Description</b>	
<b>Targets</b>	 coronavirus
<b>Assays</b>	 <b>Extraction - Manual Extraction Process</b> <ul style="list-style-type: none"> <li>● Commercial <ul style="list-style-type: none"> <li>○ Kit Manufacturer: <i>GeneProof</i></li> <li>○ Kit Type: <i>PathogenFree RNA Isolation Kit</i></li> </ul> </li> </ul>  <b>Amplification - GeneProof - croBEE Real-Time PCR System</b> <ul style="list-style-type: none"> <li>● Commercial <ul style="list-style-type: none"> <li>○ Kit Manufacturer: <i>GeneProof</i></li> <li>○ Kit Type: <i>SARS-CoV-2 PCR Kit</i></li> <li>○ Kit Version: <i>GP</i></li> </ul> </li> </ul>

## Further Programme Details

Number of Participants	300
Number of Countries	35
Number of Respondents	268
Number of Datasets Submitted	451
Qualitative Results Returned	451 (100.0%)

## EQA Programme Aims


To assess laboratories in the molecular detection of SARS-CoV-2 at clinically appropriate levels, near the limit of detection of the assay as well as the specificity of molecular assay in the presence of other non-SARS coronaviruses.

<b>Individual Report</b>		<b>QCMD 2020 SARS-CoV-2 EQA Programme</b>				
<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023

### Feedback and Enquiries

Participants are encouraged to read the QCMD Participants' Manual, which can be downloaded from the QCMD website.

Any enquiries should be submitted through the 'Contact Us' form that you can find in the 'Help' section of your QCMD (ITEMS) Participant Profile Area.

<b>Individual Report</b>		<b>QCMD 2020 SARS-CoV-2 EQA Programme</b>			 <small>Quality Control for Molecular Diagnostics</small>	
<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023

Panel member analysis is separated into CORE samples followed by EDUCATIONAL samples.

## Additional Core Samples Information

The following section has been categorised as shown below:

Core ► Qualitative

### Individual Panel Member Analysis (Qualitative)


Qualitative analysis for each panel member is provided in relation to your EQA assessment group. EQA assessment groups are established using the molecular workflow information reported by all participants within this EQA challenge / distribution. The principal level of assessment is at the individual method level which is defined based on your reported “amplification/detection method” and other laboratories using the same or similar amplification/detection methods.

To allow meaningful assessment at the individual method level the EQA assessment group must consist of 5 or more datasets. If there are not sufficient datasets at the individual method level then your results will be included within a higher EQA assessment group based on whether it is a commercial or in house technology/method. The highest level assessment grouping is “All” participant reported qualitative results.

A breakdown of qualitative results reported by participants on each of the panel members within this EQA challenge / distribution is provided below. You can compare your results to those within your EQA assessment group and those obtained within other EQA assessment groups or to the overall consensus for each sample within this EQA challenge / distribution.

**SCV2\_101C2-01 - Qualitative Results Breakdown**

Sample Code	Sample Content	Matrix	Sample Relationships	Detection Frequency	Sample Status	Percentage Correct (All)	
						(%)	(n)
SCV2_101C2-01	Coronavirus OC43	Transport Medium	4.0 dPCR Log10 Copies/ml	Negative	CORE	97.8	451

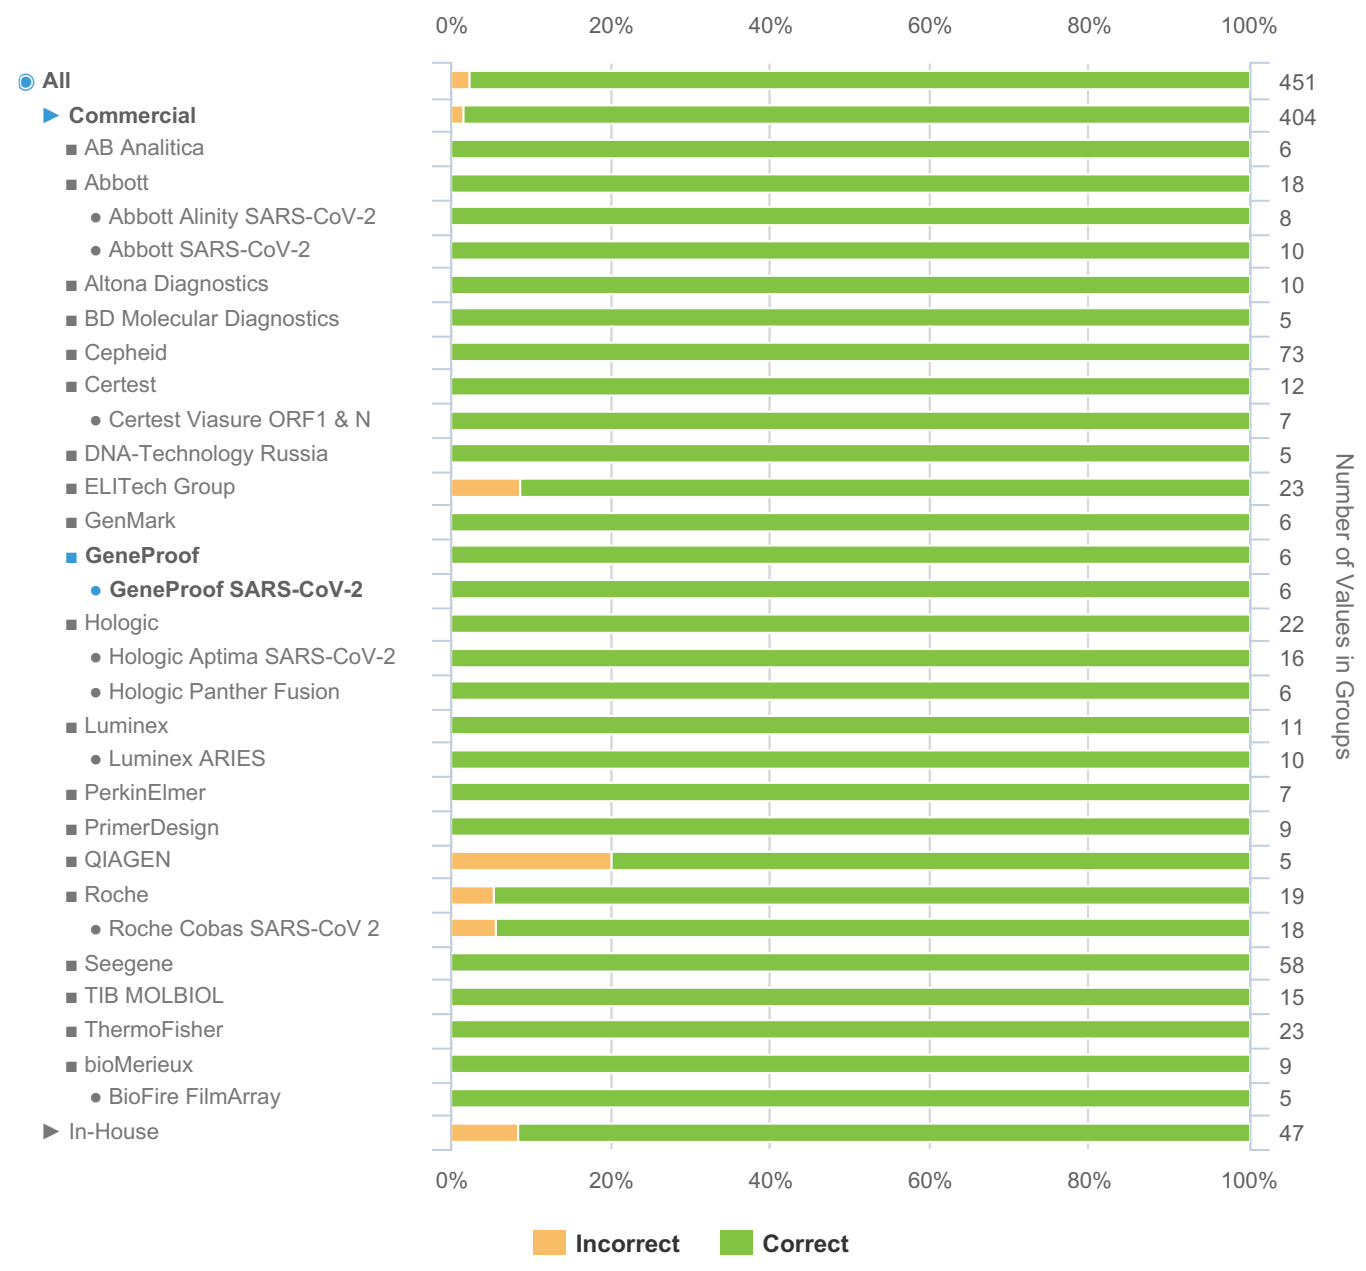

# Individual Report

# QCMD 2020 SARS-CoV-2 EQA Programme




<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory:</b> CZ023
-------------------------------------	-----------------------------	-------------------------	--------------------------------------	---------------------------	--	-----------------------------

**Groups below n=5:** AITbiotech (n=1), AITbiotech - AITbiotech abTES COVID-19 (n=1), Abacus Diagnostica (n=1), Abacus Diagnostica - Abacus Diagnostica SARS-CoV-2 (n=1), Agena Bioscience (n=1), Agena Bioscience - Agena Bioscience SARS-CoV-2 (n=1), Anatolia Geneworks (n=4), Anatolia Geneworks - Anatolia Geneworks Bosphore nCoV (n=4), AusDiagnostics (n=3), AusDiagnostics - AusDiagnostics Easy-Plex (n=1), AusDiagnostics - AusDiagnostics SARS-CoV-2 (n=2), BioMaxima (n=1), BioMaxima - BioMaxima SARS-Cov-2 (n=1), CDC (n=3), CDC - CDC SARS-CoV-2 (n=3), Certest - Certest Viasure N1 + N2 (n=4), Certest - Certest Viasure S (n=1), Convergent Technologies (n=1), Convergent Technologies - Convergys COVID 19 (n=1), Coyote Bioscience (n=1), Coyote Bioscience - Coyote Bioscience SARS-CoV-2 (n=1), Detagen Genetic Diagnostic (n=1), Detagen Genetic Diagnostic - Detagen Genetic Diagnostic SARS-CoV-2 (n=1), DiaCarta (n=2), DiaCarta - DiaCarta QuantiVirus PCR kit (n=2), DiaPro (n=1), DiaPro - DiaPro COVID-19 (n=1), DiaSorin (n=2), DiaSorin - DiaSorin Simplexa (n=2), Diagenode (n=2), Diagenode - Diagenode Real-Time PCR (n=2), Elisabeth Pharmacon (n=1), Elisabeth Pharmacon - EliGene COVID19 CONFIRM RT (n=1), Genematrix (n=2), Genematrix - Genematrix NeoPlex COVID-19 (n=2), Generon (n=1), Generon - Generon VetFinder (n=1), Genetic Signatures (n=1), Genetic Signatures - Genetic Signatures SARS-CoV-2 (n=1), Gerbion (n=3), Gerbion - Gerbion respiraScreen (n=2), Gerbion - Gerbion virella SARS-CoV-2 (n=1), Gold Standard Diagnostics (n=1), Gold Standard Diagnostics - GSD NovaPrime SARS-CoV-2 (n=1), Grifols (n=2), Grifols - Grifols Procleix SARS-CoV-2 (n=2), HybriBio Limited (n=1), HybriBio Limited - HybriBio Real-Time PCR Kit (n=1), Idil Biotech (n=1), Idil Biotech - Idil Biotech RevoDx SARS-CoV-2 (n=1), Immundiagnostik (n=2), Immundiagnostik - Immundiagnostik MutaPLEX (n=2), KH Medical (n=1), KH Medical - KH Medical RADi COVID 19 (n=1), Kogene Biotech (n=4), Kogene Biotech - Kogene Powerchek (n=4), Liferiver (n=1), Liferiver - Liferiver 2019-nCoV (n=1), Luminex - Luminex xTAG (n=1), Maccura Biotechnology (n=1), Maccura Biotechnology - Maccura SARS-CoV-2 (n=1), Mobidiag (n=1), Mobidiag - Mobidiag Novodiag (n=1), NeuMoDx (n=1), NeuMoDx - NeuMoDx SARSCoV-2 (n=1), PathoFinder (n=4), PathoFinder - PathoFinder Real Time PCR (n=1), PathoFinder - PathoFinder RealAccurate SARS-CoV-2 (n=3), PentaBase (n=1), PentaBase - PentaBase CoviDetect (n=1), Phase Scientific (n=1), Phase Scientific - Phase Scientific Covid-19 (n=1), QIAGEN - Qiagen NeuMoDx (n=1), QIAGEN - Qiagen QIAprep & amp (n=2), QIAGEN - Qiagen QIAstat-Dx (n=2), Roche - Roche LightCycler Multiplex RNA Virus (n=1), Sansure Biotech (n=1), Sansure Biotech - Sansure Biotech nCoV PCR Kit (n=1), Uni-Medica (n=1), Uni-Medica - Uni-Medica Novel Coronavirus 2019 (n=1), Vector Best (n=1), Vector Best - Vector Best SARS-CoV-2 (n=1), Vircell (n=1), Vircell - Vircell SARS-CoV-2 (n=1), YouSeq (n=2), YouSeq - YouSeq SARS CoV-2 (n=2), bioMerieux - bioMerieux R-gene SARS-CoV-2 (n=4), fast-track DIAGNOSTICS (n=2), fast-track DIAGNOSTICS - FTD real time PCR (n=2)

**Groups Rolled Up:** AB Analytica - AB Analytica REALQUALITY RQ (n=6), Altona Diagnostics - Altona Diagnostics RealStar (n=10), BD Molecular Diagnostics - BD SARS-CoV-2 (n=5), Cepheid - Cepheid Xpert SARS-CoV-2 (n=73), DNA-Technology Russia - DNA-Technology Covid-19 (n=5), ELITech Group - Elitech GeneFinder (n=23), GenMark - GenMark SARS-CoV-2 (n=6), PerkinElmer - PerkinElmer SARS-CoV-2 Real Time PCR (n=7), PrimerDesign - PrimerDesign Genesig (n=9), Seegene - Seegene Allplex SARS-CoV-2 (n=58), TIB MOLBIOL - TIB MOLBIOL LightMix (n=15), ThermoFisher - ThermoFisher TaqPath COVID-19 (n=23), In-House - Real-time In-House PCR (n=47)

**SCV2\_101C2-02 - Qualitative Results Breakdown**

Sample Code	Sample Content	Matrix	Sample Relationships	Detection Frequency	Sample Status	Percentage Correct (All)	
						(%)	(n)
SCV2_101C2-02	SARS-CoV-2	Transport Medium	3.27 dPCR Log10 Copies/ml (DS1_1)	Frequently Detected	CORE	98.7	451

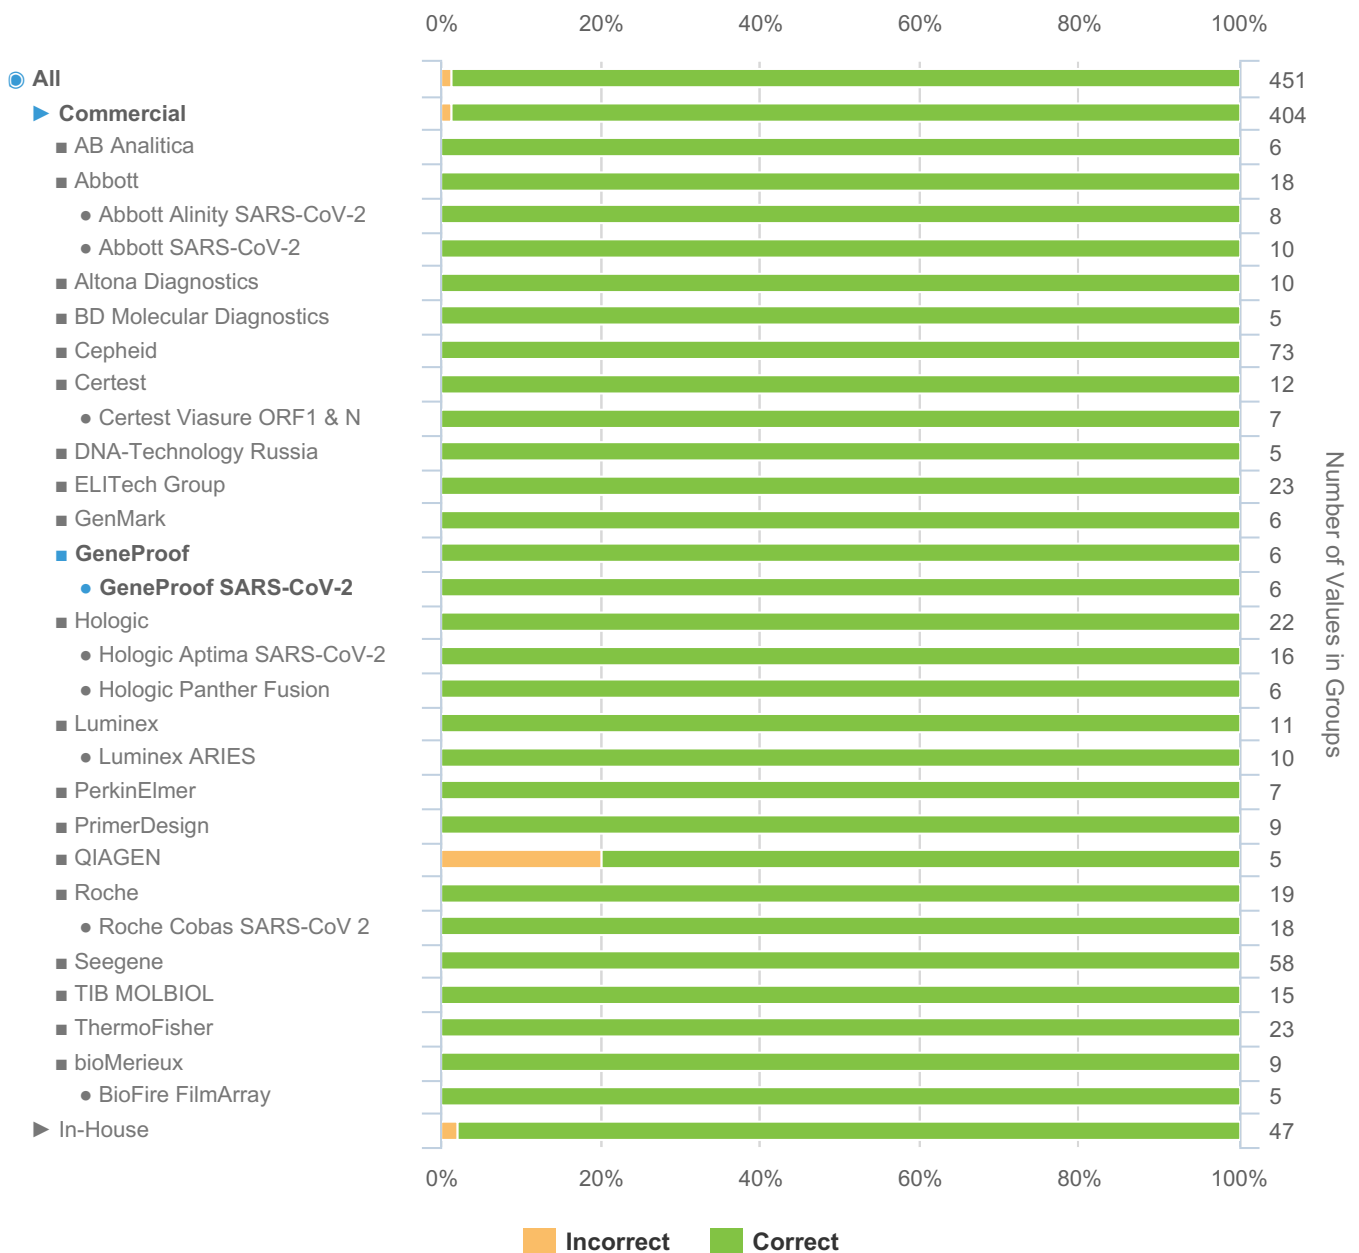



# Individual Report

# QCMD 2020 SARS-CoV-2 EQA Programme




<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory:</b> CZ023
-------------------------------------	-----------------------------	-------------------------	--------------------------------------	---------------------------	--	-----------------------------

**Groups below n=5:** AITbiotech (n=1), AITbiotech - AITbiotech abTES COVID-19 (n=1), Abacus Diagnostica (n=1), Abacus Diagnostica - Abacus Diagnostica SARS-CoV-2 (n=1), Agena Bioscience (n=1), Agena Bioscience - Agena Bioscience SARS-CoV-2 (n=1), Anatolia Geneworks (n=4), Anatolia Geneworks - Anatolia Geneworks Bosphore nCoV (n=4), AusDiagnostics (n=3), AusDiagnostics - AusDiagnostics Easy-Plex (n=1), AusDiagnostics - AusDiagnostics SARS-CoV-2 (n=2), BioMaxima (n=1), BioMaxima - BioMaxima SARS-Cov-2 (n=1), CDC (n=3), CDC - CDC SARS-CoV-2 (n=3), Certest - Certest Viasure N1 + N2 (n=4), Certest - Certest Viasure S (n=1), Convergent Technologies (n=1), Convergent Technologies - Convergys COVID 19 (n=1), Coyote Bioscience (n=1), Coyote Bioscience - Coyote Bioscience SARS-CoV-2 (n=1), Detagen Genetic Diagnostic (n=1), Detagen Genetic Diagnostic - Detagen Genetic Diagnostic SARS-CoV-2 (n=1), DiaCarta (n=2), DiaCarta - DiaCarta QuantiVirus PCR kit (n=2), DiaPro (n=1), DiaPro - DiaPro COVID-19 (n=1), DiaSorin (n=2), DiaSorin - DiaSorin Simplexa (n=2), Diagenode (n=2), Diagenode - Diagenode Real-Time PCR (n=2), Elisabeth Pharmacon (n=1), Elisabeth Pharmacon - EliGene COVID19 CONFIRM RT (n=1), Genematrix (n=2), Genematrix - Genematrix NeoPlex COVID-19 (n=2), Generon (n=1), Generon - Generon VetFinder (n=1), Genetic Signatures (n=1), Genetic Signatures - Genetic Signatures SARS-CoV-2 (n=1), Gerbion (n=3), Gerbion - Gerbion respiraScreen (n=2), Gerbion - Gerbion virella SARS-CoV-2 (n=1), Gold Standard Diagnostics (n=1), Gold Standard Diagnostics - GSD NovaPrime SARS-CoV-2 (n=1), Grifols (n=2), Grifols - Grifols Procleix SARS-CoV-2 (n=2), HybriBio Limited (n=1), HybriBio Limited - HybriBio Real-Time PCR Kit (n=1), Idil Biotech (n=1), Idil Biotech - Idil Biotech RevoDx SARS-CoV-2 (n=1), Immundiagnostik (n=2), Immundiagnostik - Immundiagnostik MutaPLEX (n=2), KH Medical (n=1), KH Medical - KH Medical RADi COVID 19 (n=1), Kogene Biotech (n=4), Kogene Biotech - Kogene Powerchek (n=4), Liferiver (n=1), Liferiver - Liferiver 2019-nCoV (n=1), Luminex - Luminex xTAG (n=1), Maccura Biotechnology (n=1), Maccura Biotechnology - Maccura SARS-CoV-2 (n=1), Mobidiag (n=1), Mobidiag - Mobidiag Novodiag (n=1), NeuMoDx (n=1), NeuMoDx - NeuMoDx SARSCoV-2 (n=1), PathoFinder (n=4), PathoFinder - PathoFinder Real Time PCR (n=1), PathoFinder - PathoFinder RealAccurate SARS-CoV-2 (n=3), PentaBase (n=1), PentaBase - PentaBase CoviDetect (n=1), Phase Scientific (n=1), Phase Scientific - Phase Scientific Covid-19 (n=1), QIAGEN - Qiagen NeuMoDx (n=1), QIAGEN - Qiagen QIAprep & amp (n=2), QIAGEN - Qiagen QIAstat-Dx (n=2), Roche - Roche LightCycler Multiplex RNA Virus (n=1), Sansure Biotech (n=1), Sansure Biotech - Sansure Biotech nCoV PCR Kit (n=1), Uni-Medica (n=1), Uni-Medica - Uni-Medica Novel Coronavirus 2019 (n=1), Vector Best (n=1), Vector Best - Vector Best SARS-CoV-2 (n=1), Vircell (n=1), Vircell - Vircell SARS-CoV-2 (n=1), YouSeq (n=2), YouSeq - YouSeq SARS CoV-2 (n=2), bioMerieux - bioMerieux R-gene SARS-CoV-2 (n=4), fast-track DIAGNOSTICS (n=2), fast-track DIAGNOSTICS - FTD real time PCR (n=2)

**Groups Rolled Up:** AB Analytica - AB Analytica REALQUALITY RQ (n=6), Altona Diagnostics - Altona Diagnostics RealStar (n=10), BD Molecular Diagnostics - BD SARS-CoV-2 (n=5), Cepheid - Cepheid Xpert SARS-CoV-2 (n=73), DNA-Technology Russia - DNA-Technology Covid-19 (n=5), ELITech Group - Elitech GeneFinder (n=23), GenMark - GenMark SARS-CoV-2 (n=6), PerkinElmer - PerkinElmer SARS-CoV-2 Real Time PCR (n=7), PrimerDesign - PrimerDesign Genesig (n=9), Seegene - Seegene Allplex SARS-CoV-2 (n=58), TIB MOLBIOL - TIB MOLBIOL LightMix (n=15), ThermoFisher - ThermoFisher TaqPath COVID-19 (n=23), In-House - Real-time In-House PCR (n=47)

**SCV2\_101C2-03 - Qualitative Results Breakdown**

Sample Code	Sample Content	Matrix	Sample Relationships	Detection Frequency	Sample Status	Percentage Correct (All)	
						(%)	(n)
SCV2_101C2-03	SARS-CoV-2	Transport Medium	2.48 dPCR Log10 Copies/ml (D1, DS1_2)	Detected	CORE	93.1	451

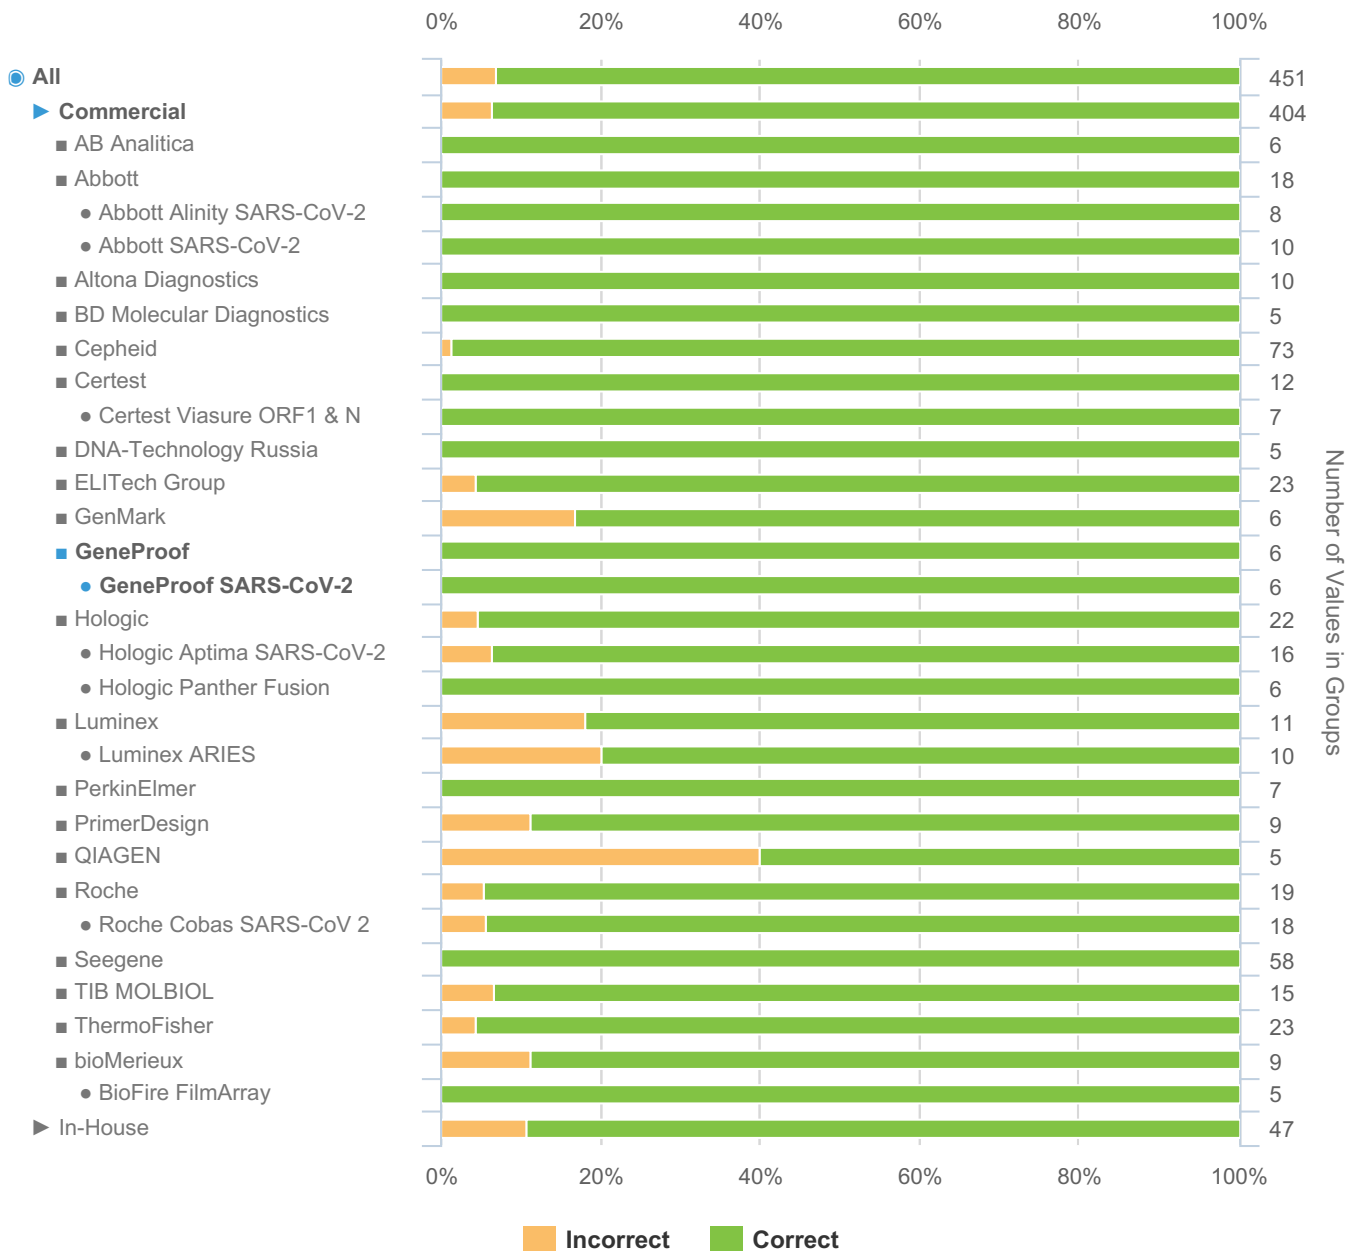

# Individual Report

# QCMD 2020 SARS-CoV-2 EQA Programme




<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023
-------------------------------------	-----------------------------	-------------------------	--------------------------------------	---------------------------	--	----------------------------

**Groups below n=5:** AITbiotech (n=1), AITbiotech - AITbiotech abTES COVID-19 (n=1), Abacus Diagnostica (n=1), Abacus Diagnostica - Abacus Diagnostica SARS-CoV-2 (n=1), Agena Bioscience (n=1), Agena Bioscience - Agena Bioscience SARS-CoV-2 (n=1), Anatolia Geneworks (n=4), Anatolia Geneworks - Anatolia Geneworks Bosphore nCoV (n=4), AusDiagnostics (n=3), AusDiagnostics - AusDiagnostics Easy-Plex (n=1), AusDiagnostics - AusDiagnostics SARS-CoV-2 (n=2), BioMaxima (n=1), BioMaxima - BioMaxima SARS-Cov-2 (n=1), CDC (n=3), CDC - CDC SARS-CoV-2 (n=3), Certest - Certest Viasure N1 + N2 (n=4), Certest - Certest Viasure S (n=1), Convergent Technologies (n=1), Convergent Technologies - Convergys COVID 19 (n=1), Coyote Bioscience (n=1), Coyote Bioscience - Coyote Bioscience SARS-CoV-2 (n=1), Detagen Genetic Diagnostic (n=1), Detagen Genetic Diagnostic - Detagen Genetic Diagnostic SARS-CoV-2 (n=1), DiaCarta (n=2), DiaCarta - DiaCarta QuantiVirus PCR kit (n=2), DiaPro (n=1), DiaPro - DiaPro COVID-19 (n=1), DiaSorin (n=2), DiaSorin - DiaSorin Simplexa (n=2), Diagenode (n=2), Diagenode - Diagenode Real-Time PCR (n=2), Elisabeth Pharmacon (n=1), Elisabeth Pharmacon - EliGene COVID19 CONFIRM RT (n=1), Genematrix (n=2), Genematrix - Genematrix NeoPlex COVID-19 (n=2), Generon (n=1), Generon - Generon VetFinder (n=1), Genetic Signatures (n=1), Genetic Signatures - Genetic Signatures SARS-CoV-2 (n=1), Gerbion (n=3), Gerbion - Gerbion respiraScreen (n=2), Gerbion - Gerbion virella SARS-CoV-2 (n=1), Gold Standard Diagnostics (n=1), Gold Standard Diagnostics - GSD NovaPrime SARS-CoV-2 (n=1), Grifols (n=2), Grifols - Grifols Procleix SARS-CoV-2 (n=2), HybriBio Limited (n=1), HybriBio Limited - HybriBio Real-Time PCR Kit (n=1), Idil Biotech (n=1), Idil Biotech - Idil Biotech RevoDx SARS-CoV-2 (n=1), Immundiagnostik (n=2), Immundiagnostik - Immundiagnostik MutaPLEX (n=2), KH Medical (n=1), KH Medical - KH Medical RADi COVID 19 (n=1), Kogene Biotech (n=4), Kogene Biotech - Kogene Powerchek (n=4), Liferiver (n=1), Liferiver - Liferiver 2019-nCoV (n=1), Luminex - Luminex xTAG (n=1), Maccura Biotechnology (n=1), Maccura Biotechnology - Maccura SARS-CoV-2 (n=1), Mobidiag (n=1), Mobidiag - Mobidiag Novodiag (n=1), NeuMoDx (n=1), NeuMoDx - NeuMoDx SARSCoV-2 (n=1), PathoFinder (n=4), PathoFinder - PathoFinder Real Time PCR (n=1), PathoFinder - PathoFinder RealAccurate SARS-CoV-2 (n=3), PentaBase (n=1), PentaBase - PentaBase CoviDetect (n=1), Phase Scientific (n=1), Phase Scientific - Phase Scientific Covid-19 (n=1), QIAGEN - Qiagen NeuMoDx (n=1), QIAGEN - Qiagen QIAprep & amp (n=2), QIAGEN - Qiagen QIAstat-Dx (n=2), Roche - Roche LightCycler Multiplex RNA Virus (n=1), Sansure Biotech (n=1), Sansure Biotech - Sansure Biotech nCoV PCR Kit (n=1), Uni-Medica (n=1), Uni-Medica - Uni-Medica Novel Coronavirus 2019 (n=1), Vector Best (n=1), Vector Best - Vector Best SARS-CoV-2 (n=1), Vircell (n=1), Vircell - Vircell SARS-CoV-2 (n=1), YouSeq (n=2), YouSeq - YouSeq SARS CoV-2 (n=2), bioMerieux - bioMerieux R-gene SARS-CoV-2 (n=4), fast-track DIAGNOSTICS (n=2), fast-track DIAGNOSTICS - FTD real time PCR (n=2)

**Groups Rolled Up:** AB Analytica - AB Analytica REALQUALITY RQ (n=6), Altona Diagnostics - Altona Diagnostics RealStar (n=10), BD Molecular Diagnostics - BD SARS-CoV-2 (n=5), Cepheid - Cepheid Xpert SARS-CoV-2 (n=73), DNA-Technology Russia - DNA-Technology Covid-19 (n=5), ELITech Group - Elitech GeneFinder (n=23), GenMark - GenMark SARS-CoV-2 (n=6), PerkinElmer - PerkinElmer SARS-CoV-2 Real Time PCR (n=7), PrimerDesign - PrimerDesign Genesig (n=9), Seegene - Seegene Allplex SARS-CoV-2 (n=58), TIB MOLBIOL - TIB MOLBIOL LightMix (n=15), ThermoFisher - ThermoFisher TaqPath COVID-19 (n=23), In-House - Real-time In-House PCR (n=47)

**SCV2\_101C2-04 - Qualitative Results Breakdown**

Sample Code	Sample Content	Matrix	Sample Relationships	Detection Frequency	Sample Status	Percentage Correct (All)	
						(%)	(n)
SCV2_101C2-04	SARS-CoV-2	Transport Medium	2.48 dPCR Log10 Copies/ml (D1, DS1_2)	Detected	CORE	93.6	451

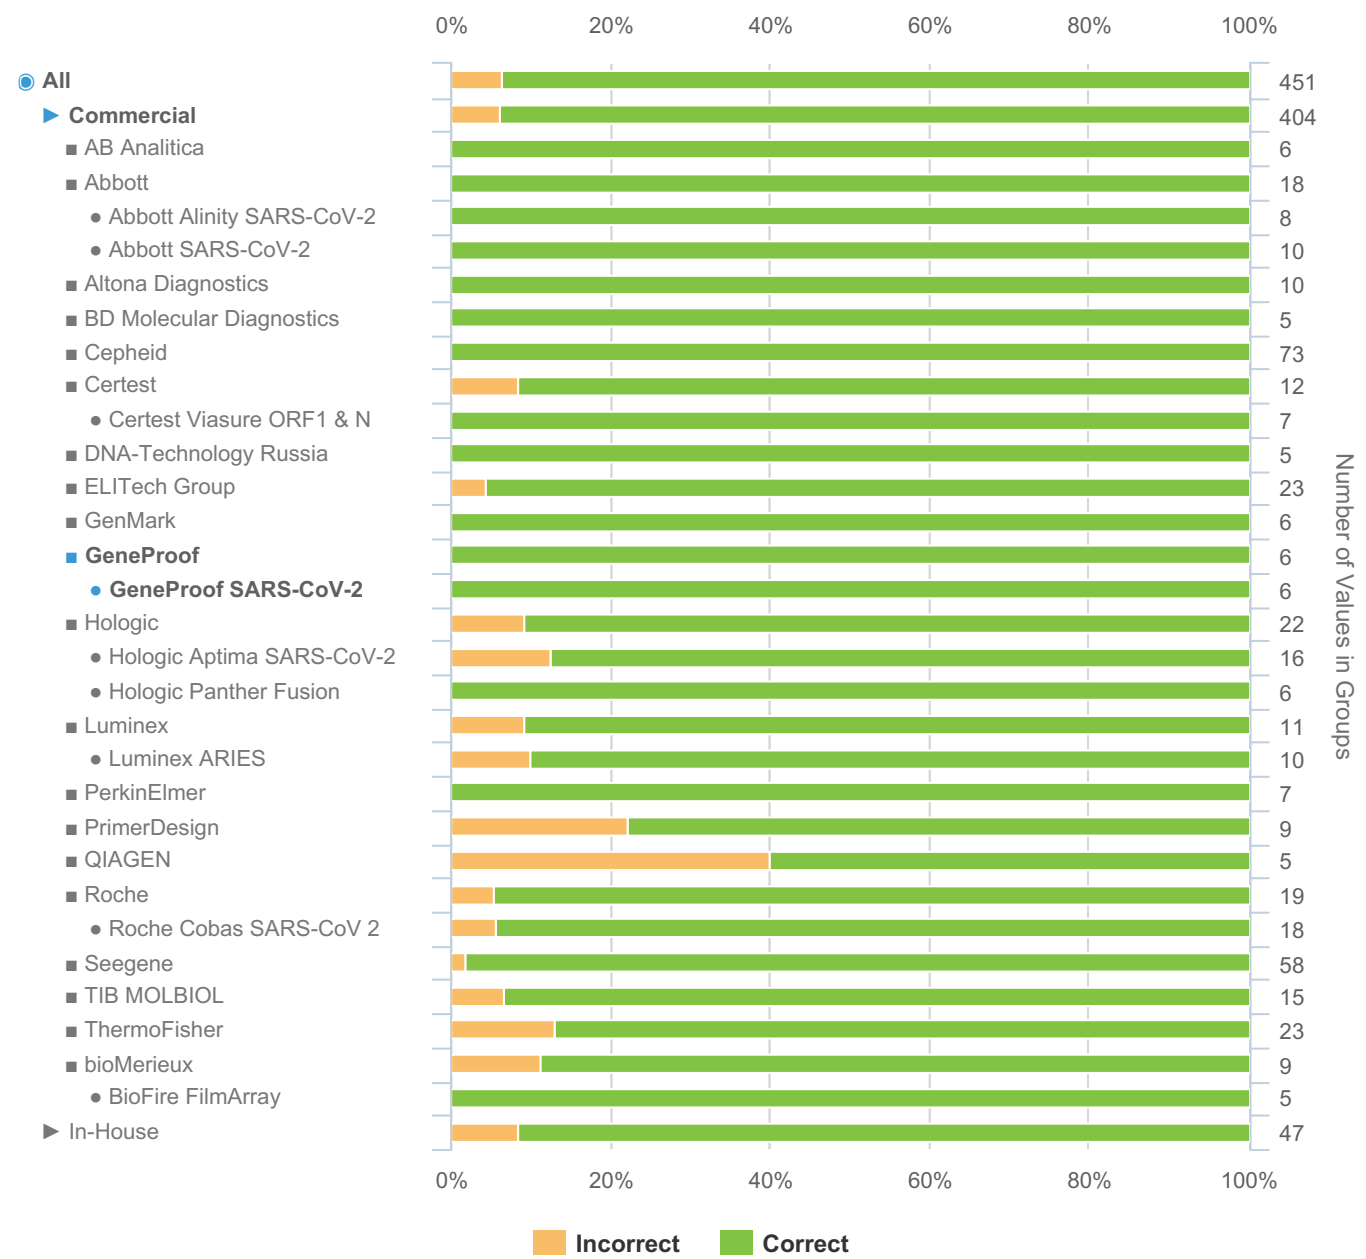

# Individual Report

# QCMD 2020 SARS-CoV-2 EQA Programme




<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023
-------------------------------------	-----------------------------	-------------------------	--------------------------------------	---------------------------	--	----------------------------

**Groups below n=5:** AITbiotech (n=1), AITbiotech - AITbiotech abTES COVID-19 (n=1), Abacus Diagnostica (n=1), Abacus Diagnostica - Abacus Diagnostica SARS-CoV-2 (n=1), Agena Bioscience (n=1), Agena Bioscience - Agena Bioscience SARS-CoV-2 (n=1), Anatolia Geneworks (n=4), Anatolia Geneworks - Anatolia Geneworks Bosphore nCoV (n=4), AusDiagnostics (n=3), AusDiagnostics - AusDiagnostics Easy-Plex (n=1), AusDiagnostics - AusDiagnostics SARS-CoV-2 (n=2), BioMaxima (n=1), BioMaxima - BioMaxima SARS-Cov-2 (n=1), CDC (n=3), CDC - CDC SARS-CoV-2 (n=3), Certest - Certest Viasure N1 + N2 (n=4), Certest - Certest Viasure S (n=1), Convergent Technologies (n=1), Convergent Technologies - Convergys COVID 19 (n=1), Coyote Bioscience (n=1), Coyote Bioscience - Coyote Bioscience SARS-CoV-2 (n=1), Detagen Genetic Diagnostic (n=1), Detagen Genetic Diagnostic - Detagen Genetic Diagnostic SARS-CoV-2 (n=1), DiaCarta (n=2), DiaCarta - DiaCarta QuantiVirus PCR kit (n=2), DiaPro (n=1), DiaPro - DiaPro COVID-19 (n=1), DiaSorin (n=2), DiaSorin - DiaSorin Simplexa (n=2), Diagenode (n=2), Diagenode - Diagenode Real-Time PCR (n=2), Elisabeth Pharmacon (n=1), Elisabeth Pharmacon - EliGene COVID19 CONFIRM RT (n=1), Genematrix (n=2), Genematrix - Genematrix NeoPlex COVID-19 (n=2), Generon (n=1), Generon - Generon VetFinder (n=1), Genetic Signatures (n=1), Genetic Signatures - Genetic Signatures SARS-CoV-2 (n=1), Gerbion (n=3), Gerbion - Gerbion respiraScreen (n=2), Gerbion - Gerbion virella SARS-CoV-2 (n=1), Gold Standard Diagnostics (n=1), Gold Standard Diagnostics - GSD NovaPrime SARS-CoV-2 (n=1), Grifols (n=2), Grifols - Grifols Procleix SARS-CoV-2 (n=2), HybriBio Limited (n=1), HybriBio Limited - HybriBio Real-Time PCR Kit (n=1), Idil Biotech (n=1), Idil Biotech - Idil Biotech RevoDx SARS-CoV-2 (n=1), Immundiagnostik (n=2), Immundiagnostik - Immundiagnostik MutaPLEX (n=2), KH Medical (n=1), KH Medical - KH Medical RADi COVID 19 (n=1), Kogene Biotech (n=4), Kogene Biotech - Kogene Powerchek (n=4), Liferiver (n=1), Liferiver - Liferiver 2019-nCoV (n=1), Luminex - Luminex xTAG (n=1), Maccura Biotechnology (n=1), Maccura Biotechnology - Maccura SARS-CoV-2 (n=1), Mobidiag (n=1), Mobidiag - Mobidiag Novodiag (n=1), NeuMoDx (n=1), NeuMoDx - NeuMoDx SARSCoV-2 (n=1), PathoFinder (n=4), PathoFinder - PathoFinder Real Time PCR (n=1), PathoFinder - PathoFinder RealAccurate SARS-CoV-2 (n=3), PentaBase (n=1), PentaBase - PentaBase CoviDetect (n=1), Phase Scientific (n=1), Phase Scientific - Phase Scientific Covid-19 (n=1), QIAGEN - Qiagen NeuMoDx (n=1), QIAGEN - Qiagen QIAprep & amp (n=2), QIAGEN - Qiagen QIAstat-Dx (n=2), Roche - Roche LightCycler Multiplex RNA Virus (n=1), Sansure Biotech (n=1), Sansure Biotech - Sansure Biotech nCoV PCR Kit (n=1), Uni-Medica (n=1), Uni-Medica - Uni-Medica Novel Coronavirus 2019 (n=1), Vector Best (n=1), Vector Best - Vector Best SARS-CoV-2 (n=1), Vircell (n=1), Vircell - Vircell SARS-CoV-2 (n=1), YouSeq (n=2), YouSeq - YouSeq SARS CoV-2 (n=2), bioMerieux - bioMerieux R-gene SARS-CoV-2 (n=4), fast-track DIAGNOSTICS (n=2), fast-track DIAGNOSTICS - FTD real time PCR (n=2)

**Groups Rolled Up:** AB Analytica - AB Analytica REALQUALITY RQ (n=6), Altona Diagnostics - Altona Diagnostics RealStar (n=10), BD Molecular Diagnostics - BD SARS-CoV-2 (n=5), Cepheid - Cepheid Xpert SARS-CoV-2 (n=73), DNA-Technology Russia - DNA-Technology Covid-19 (n=5), ELITech Group - Elitech GeneFinder (n=23), GenMark - GenMark SARS-CoV-2 (n=6), PerkinElmer - PerkinElmer SARS-CoV-2 Real Time PCR (n=7), PrimerDesign - PrimerDesign Genesig (n=9), Seegene - Seegene Allplex SARS-CoV-2 (n=58), TIB MOLBIOL - TIB MOLBIOL LightMix (n=15), ThermoFisher - ThermoFisher TaqPath COVID-19 (n=23), In-House - Real-time In-House PCR (n=47)

**SCV2\_101C2-05 - Qualitative Results Breakdown**

Sample Code	Sample Content	Matrix	Sample Relationships	Detection Frequency	Sample Status	Percentage Correct (All)	
						(%)	(n)
SCV2_101C2-05	Coronavirus Negative	Transport Medium		Negative	CORE	99.1	451

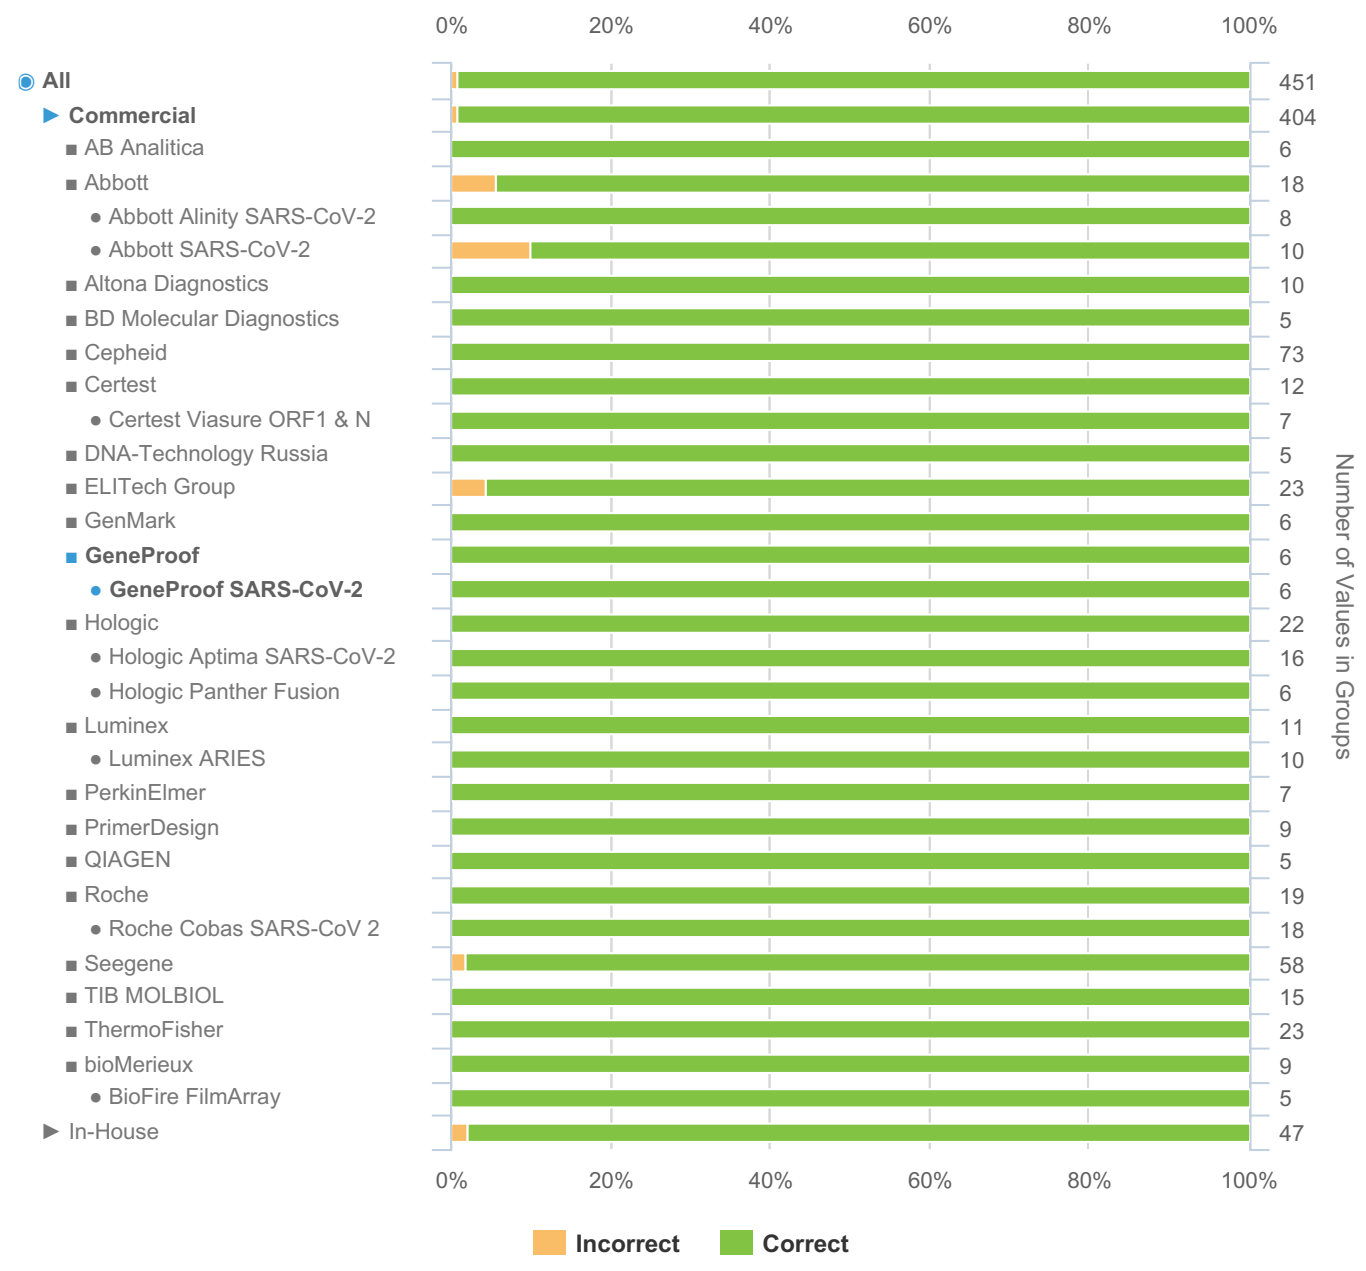

# Individual Report

# QCMD 2020 SARS-CoV-2 EQA Programme



<b>Catalogue Code:</b> QAV204215	<b>Ref Code:</b> SCV2_20	<b>Challenge:</b> C2	<b>Analysis Type:</b> Qualitative	<b>Dataset:</b> 414167	<b>Report UID:</b> 2677/414167/3130	<b>Laboratory</b> CZ023
-------------------------------------	-----------------------------	-------------------------	--------------------------------------	---------------------------	--	----------------------------

**Groups below n=5:** AITbiotech (n=1), AITbiotech - AITbiotech abTES COVID-19 (n=1), Abacus Diagnostica (n=1), Abacus Diagnostica - Abacus Diagnostica SARS-CoV-2 (n=1), Agena Bioscience (n=1), Agena Bioscience - Agena Bioscience SARS-CoV-2 (n=1), Anatolia Geneworks (n=4), Anatolia Geneworks - Anatolia Geneworks Bosphore nCoV (n=4), AusDiagnostics (n=3), AusDiagnostics - AusDiagnostics Easy-Plex (n=1), AusDiagnostics - AusDiagnostics SARS-CoV-2 (n=2), BioMaxima (n=1), BioMaxima - BioMaxima SARS-Cov-2 (n=1), CDC (n=3), CDC - CDC SARS-CoV-2 (n=3), Certest - Certest Viasure N1 + N2 (n=4), Certest - Certest Viasure S (n=1), Convergent Technologies (n=1), Convergent Technologies - Convergys COVID 19 (n=1), Coyote Bioscience (n=1), Coyote Bioscience - Coyote Bioscience SARS-CoV-2 (n=1), Detagen Genetic Diagnostic (n=1), Detagen Genetic Diagnostic - Detagen Genetic Diagnostic SARS-CoV-2 (n=1), DiaCarta (n=2), DiaCarta - DiaCarta QuantiVirus PCR kit (n=2), DiaPro (n=1), DiaPro - DiaPro COVID-19 (n=1), DiaSorin (n=2), DiaSorin - DiaSorin Simplexa (n=2), Diagenode (n=2), Diagenode - Diagenode Real-Time PCR (n=2), Elisabeth Pharmacon (n=1), Elisabeth Pharmacon - EliGene COVID19 CONFIRM RT (n=1), Genematrix (n=2), Genematrix - Genematrix NeoPlex COVID-19 (n=2), Generon (n=1), Generon - Generon VetFinder (n=1), Genetic Signatures (n=1), Genetic Signatures - Genetic Signatures SARS-CoV-2 (n=1), Gerbion (n=3), Gerbion - Gerbion respiraScreen (n=2), Gerbion - Gerbion virella SARS-CoV-2 (n=1), Gold Standard Diagnostics (n=1), Gold Standard Diagnostics - GSD NovaPrime SARS-CoV-2 (n=1), Grifols (n=2), Grifols - Grifols Procleix SARS-CoV-2 (n=2), HybriBio Limited (n=1), HybriBio Limited - HybriBio Real-Time PCR Kit (n=1), Idil Biotech (n=1), Idil Biotech - Idil Biotech RevoDx SARS-CoV-2 (n=1), Immundiagnostik (n=2), Immundiagnostik - Immundiagnostik MutaPLEX (n=2), KH Medical (n=1), KH Medical - KH Medical RADi COVID 19 (n=1), Kogene Biotech (n=4), Kogene Biotech - Kogene Powerchek (n=4), Liferiver (n=1), Liferiver - Liferiver 2019-nCoV (n=1), Luminex - Luminex xTAG (n=1), Maccura Biotechnology (n=1), Maccura Biotechnology - Maccura SARS-CoV-2 (n=1), Mobidiag (n=1), Mobidiag - Mobidiag Novodiag (n=1), NeuMoDx (n=1), NeuMoDx - NeuMoDx SARSCoV-2 (n=1), PathoFinder (n=4), PathoFinder - PathoFinder Real Time PCR (n=1), PathoFinder - PathoFinder RealAccurate SARS-CoV-2 (n=3), PentaBase (n=1), PentaBase - PentaBase CoviDetect (n=1), Phase Scientific (n=1), Phase Scientific - Phase Scientific Covid-19 (n=1), QIAGEN - Qiagen NeuMoDx (n=1), QIAGEN - Qiagen QIAprep & amp (n=2), QIAGEN - Qiagen QIAstat-Dx (n=2), Roche - Roche LightCycler Multiplex RNA Virus (n=1), Sansure Biotech (n=1), Sansure Biotech - Sansure Biotech nCoV PCR Kit (n=1), Uni-Medica (n=1), Uni-Medica - Uni-Medica Novel Coronavirus 2019 (n=1), Vector Best (n=1), Vector Best - Vector Best SARS-CoV-2 (n=1), Vircell (n=1), Vircell - Vircell SARS-CoV-2 (n=1), YouSeq (n=2), YouSeq - YouSeq SARS CoV-2 (n=2), bioMerieux - bioMerieux R-gene SARS-CoV-2 (n=4), fast-track DIAGNOSTICS (n=2), fast-track DIAGNOSTICS - FTD real time PCR (n=2)

**Groups Rolled Up:** AB Analytica - AB Analytica REALQUALITY RQ (n=6), Altona Diagnostics - Altona Diagnostics RealStar (n=10), BD Molecular Diagnostics - BD SARS-CoV-2 (n=5), Cepheid - Cepheid Xpert SARS-CoV-2 (n=73), DNA-Technology Russia - DNA-Technology Covid-19 (n=5), ELITech Group - Elitech GeneFinder (n=23), GenMark - GenMark SARS-CoV-2 (n=6), PerkinElmer - PerkinElmer SARS-CoV-2 Real Time PCR (n=7), PrimerDesign - PrimerDesign Genesig (n=9), Seegene - Seegene Allplex SARS-CoV-2 (n=58), TIB MOLBIOL - TIB MOLBIOL LightMix (n=15), ThermoFisher - ThermoFisher TaqPath COVID-19 (n=23), In-House - Real-time In-House PCR (n=47)

**QCMD © 2020.** The QCMD EQA programme samples, associated reports and data generated during this programme are intended for External Quality Assessment (EQA) and Proficiency Testing (PT) purposes only. QCMD operates according to a strict Code of Practice which is in line with ISO/IEC 17043 and associated standards. Data reported in QCMD programmes is representative of a laboratory's standard diagnostic testing protocols irrespective of the technology they use. The data provided in the reports are based on technical information provided by the individual laboratories as part of the assessment process, as such it does not constitute a formal technology method comparison. All text and images produced by QCMD are the property of QCMD unless otherwise stated.

The reproduction and use of these materials is not permitted without the express written consent of QCMD. The use of the information provided in QCMD reports for commercial purposes is strictly prohibited.